



Sigma Scientific LLC.

Custom Y-Tube Measurements Form

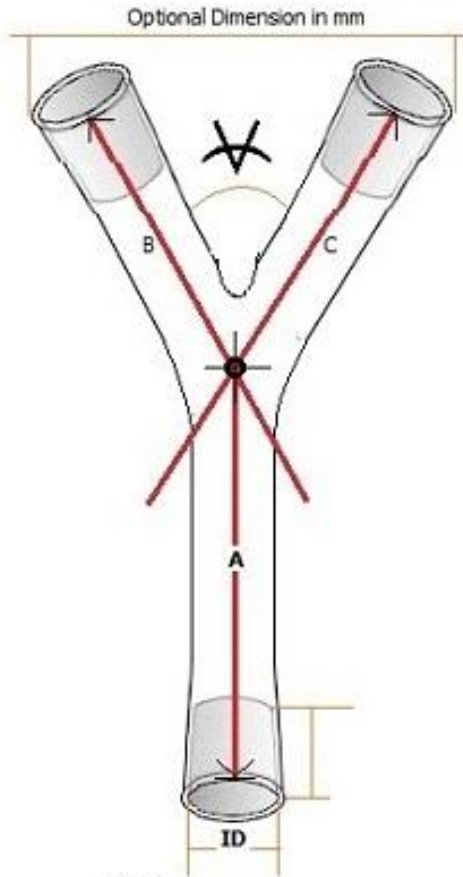


Both the External Odor Source (OSE) and the Specimen Adaptors (SA) are standard sizes dependent on Ground Joint used.

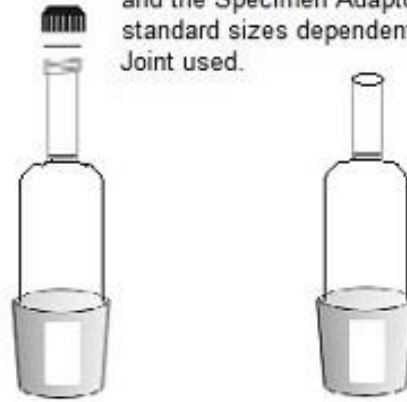

Inline Odor Source Chamber (Custom)

ID of Odor Chamber = _____ mm

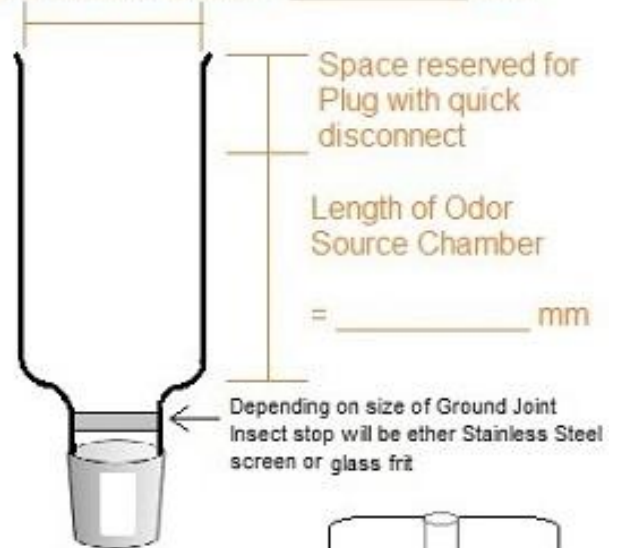

Plug with quick disconnect custom made to Chamber size

